

Assessment of Gamma Camera SPECT Resolution using Developed Quality Control Phantom

Mohamed E. M. Gar-el-nabi¹, Wadah M. Ali², Mohammed A. Ali Omer^{1,3}, Ghada A. Edam¹

¹College of Medical Radiologic Science, Sudan University of Science and Technology, Khartoum-Sudan

²College of Radiological Science and Nuclear Medicine Technology, The National Ribat University, Khartoum-Sudan

³College of Applied Medical Science, Department of Radiologic Technology, Qassim University, Buraidah-KSA

Abstract: The aim of this study; was to developed and designs an indigenous quality control phantom QCP to be used for gamma camera resolution QC test which installed at Royal Care hospital (RCH) and Radiation & Isotopes Center of Khartoum (RICK), as well to compare its performance relative to the standard QC phantom recommended by National Electronic Manufacture Association NEMA. The phantom has been designed based on the parameters and specifications recommended by NEMA with specific indigenous designing in view of utilizing local cheap material such as Perspex and wires lead and geometrical engineering. The comparative QC assessment for RCH and RICK revealed that: for RCH and RICK the resolution was 94.0% and 89.5% respectively which was dependant on the minimum object size resolved in the designed phantom (0.5 mm), while the resolution obtained by NEMA standard phantom showed 95.5% and 91.8% respectively. Quite similar resolution% has been obtained by the designed phantom depending on the object frequency (number of object/cm) i.e. number of lead wires resolved per cm², in this view the resolution was resolution was 94% and 90.3% respectively and in comparison with that obtained by NEMA phantom which was 95.5% and 91.8% respectively, the average deviation factor of the designed phantom from the standard was 1.5% - 1.9. Also the general trend of correlation between object size versus resolution showed a linear proportional equation in a form of $y = 6.59x + 47.87$ and $y = 6.64x + 43.1$ for RCH and RICK respectively with significant correlation as $R^2 = 0.98$. And for object frequency versus resolution, the equation trend was inversely according to: $y = -242.68x + 113.01$ for RCH and $y = -258.1x + 110.46$ for RICK, where x refers to object frequency and y refers to resolution%, with significant correlation as $R^2 = 1$.

Keywords: Gamma, Camera, Phantom, Resolution, Quality control

1. Introduction

Within Nuclear Medicine, image abnormalities and artifacts affecting the quality of images are well known phenomena [1]. Therefore, it is of great importance to have Quality Assurance for gamma and SPECT cameras to minimize the occurrence of these abnormalities and artifacts. National Electrical Manufacturers Association NEMA has made recommendations of routine quality control for nuclear medicine instrumentation [2]. After installation and before the camera is put into clinical use, it should undergo National Electrical Manufacturers Association (NEMA) Performance standard measurements to verify that the camera performs according to specification supplied by the manufacturer and to establish baseline conditions for all future measurements. The NEMA (NU 1-2007) Standards Publication [3] describes how to perform process and report of QC tests for gamma and SPECT cameras [2]. Often, with support from the manufacturers, all necessary phantoms can be supplied and acquisitions can be done according to NEMA standards, but Quality Assurance also requires a careful handling of the measured QC data. For optimal diagnostic use of nuclear medicine instruments it is essential that routine performance evaluation must be carried out as part of an ongoing quality assurance program. The NEMA publication (NU 1-2001) [4] is the basic recommended standard for performance evaluation and acceptance tests of scintillation cameras, however, the methodology and guidelines described is more complex than necessary for many nuclear medicine departments to use on a routine basis. The intrinsic flood

uniformity test of a gamma camera is a measure of the response of the gamma camera to a uniform flux of radiation from a point source when the collimator is removed or extrinsic flood uniformity test which assess the response of camera and collimator to uniform flux of radiation from ^{99m}Tc liquid flood phantom, which is one of the primary tests performed on the gamma cameras. Also there are two different uniformity parameters, usually measured during this test are: integral uniformity and differential uniformity. These are calculated for both the central field of view (CFOV) and useful field of view (UFOV) of the gamma camera. The integral uniformity has typical values of 2% to 4% [2]. For differential uniformity in most cases, a value of less than 3% is obtained after uniformity correction [5]. When the value for differential uniformity exceeds 3%, maintenance service should be carried out on the gamma camera [6]. Values of differential uniformity in the range 1.0% to 2.5% and values of integral uniformity in the range of 1.5% to 3.5% when the uniformity correction is applied are an indication that the system is working optimum. Generally, between 10 and 30 million count flood images are adequate for verification of non uniformity of the system, for all clinical studies. Spatial linearity is one of the parameters that influence flood field uniformity. In the ideal system, a straight line source of gamma rays should yield a straight line in the image. The NEMA protocol for measuring linearity involves the acquisition along the X and Y directions of an image from a multi-slit phantom, the same one used for the spatial resolution measurement, followed by an analysis of the line spread peak positions [7] (John et al, 2011). A deviation of the peak position from the true location of the center of the

slits is a measure of the deviation from linearity. Typically, most departments do not measure linearity separate from either spatial resolution or flood field uniformity [8]. Due to disadvantages of techniques used to measure gamma camera system linearity (removal of the collimator which may implies crystal break or deformity of lead septa of the collimator), the complexity of technique, and due to shortness/little funding for maintenance and the lack of a manufacturer independent QC-software supporting a NEMA performance standard which is considered as a major problem to perform NEMA QC tests; the researchers feel curious to develop a full suite of data handling software based upon the NEMA Standard Publication of NEMA NU-1 2007 [3] using interactive data language (IDL) program together with a developed phantom which is friendly applicable for routine gamma camera (SPECT) tests and low cost in Sudan. The fabricated phantom has been compared with the standard SPECT phantom to determine to what extent it mimics the standard one in view of QC test.

2. Materials and Method

The designed phantom has been excerpted from the phantom parameters stated by International Atomic Energy Agency DOC-602 [9], NEMA-2001[4], Ng et al, [10], Holstensson et al, [11]-[12] and Islamian et al, [13], which consists of four quadrate bars as recommended by Zanzorico et al, [14].

The frontal part of the phantom made of Perspex (42×42×10 cm) shown in Figure (1) that simulates the four quadrant bars phantom each one was 20×20 cm, which have been grooved by laser cutting bed (BCL-B series model BCL1318B china 1991). The first quadrant implies 26 grooves with dimensions of 18×0.35 cm and separated from each other by distance of 3.5mm. The second quadrant contains 30 grooves as 18 cm×3mm and each adjacent grooves was separated by distance of 3 mm, the third quadrant contains 32 grooves with dimension of 18cm × 0.25 cm separated by 2.5 mm distance, and the forth quadrant contains 32 Grooves with 18 cm× 2 mm and separated from each other by factor of 2 mm. The edge of the phantom i.e. the remaining 2 cm; a big grooves was made with dimension of 36 cm length and 5 mm width, which is used to measure the linearity of the gamma camera by measuring Modulation transfer function (MTF) of the Line Spread Function (LSF). The back part simulates the liquid flood phantom made of Perspex (42×42×1 cm) Figure (2) and has orifice 0.5 cm to be fill with a liquid radioactive material, controlling the air bubbles and insuring the homogeneity. Then some lead wires have been fabricated in smooth and fine shapes according the dimension of the grooves (18 × 0.35cm, 18×0.3 cm, 18×0.25 cm, 18× 0.2 cm and 36×0.5 cm) which then have been mounted in the relevant grooves in the front quadrants.

Then a mixture of water (1500ml) and $\text{Na}^{99\text{m}}\text{TcO}_4$ (1.3 mCi) has been flushed into the phantom via the orifice, shacked to maintain the homogeneity and air bubbles free. Then, the phantom has been put on the couch and centered to the gamma camera (Nucline Sprit model, single head SPECT-Hungarian) facing the central Field of View (CFOV) and image was acquired using count mode of 16 million counts

last for 2014 seconds at rate of 7749 count/second (cps) using the parameter of $256 \times 256 \times 16$ matrix size, body contour and full field. The method of imaging acquisition, phantom parameters and data collection was performed according to the parameters recommended by NEMA, IAEA, [14] and Ellinor et al, [2].



Figure 1: shows the frontal part of the phantom made of Perspex (42×42×10 cm) that simulates the four quadrant bars phantom each one was 20×20 cm



Figure 2: shows the back part simulates the liquid flood phantom made of Perspex (42×42×1 cm) and has orifice 0.5 cm to be fill with a liquid radioactive material

Then for all obtained images, the researcher applied their own developed mathematical IDL program to measure the resolution in percent versus frequency of object (numbers of wires/cm) and size of wires. The QC test of resolution has been carried out for two nuclear medicine departments specifically at Royal care and Radiation & Isotopes Center in Khartoum using the fabricated phantom and the reference standard one.

3. Results

The highlighted results show the obtained resolution percent versus object size in mm and the frequency (number of wires/cm) for Royal Care and Radiation & Isotopes Center hospitals Figure 1 and 2 as well these results have been compared with the reference result of QA done by the standard quadrant bars phantom Figure 3 and 4 respectively.

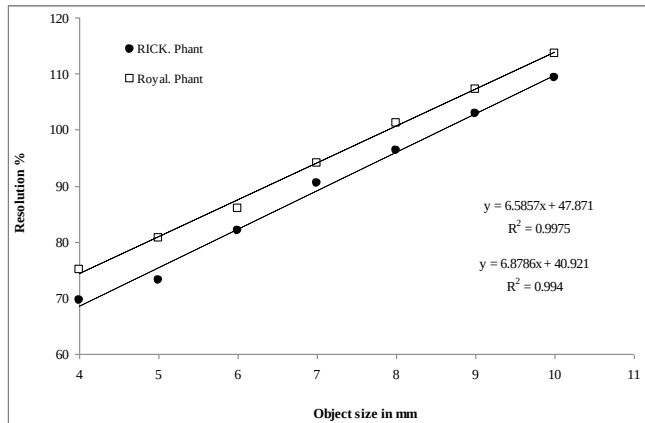


Figure 1: shows the resolution % vs. objects size for SPECT in RICK and Royal care hospitals-Khartoum Sudan using developed phantom.

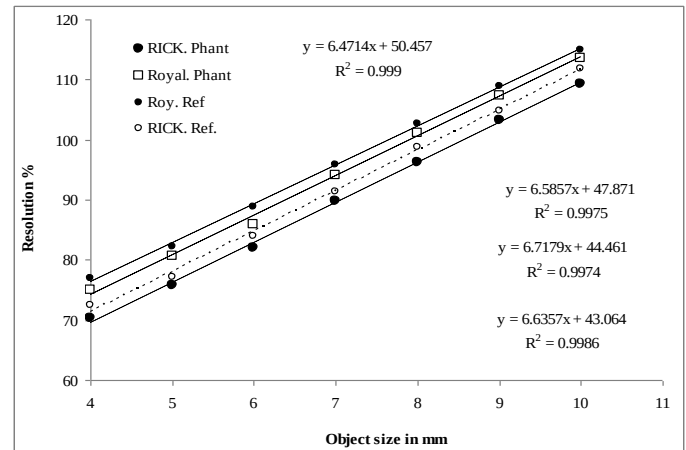


Figure 4: shows the comparison resolution% measured by phantom and the QA base line for Royal Care and RICK.

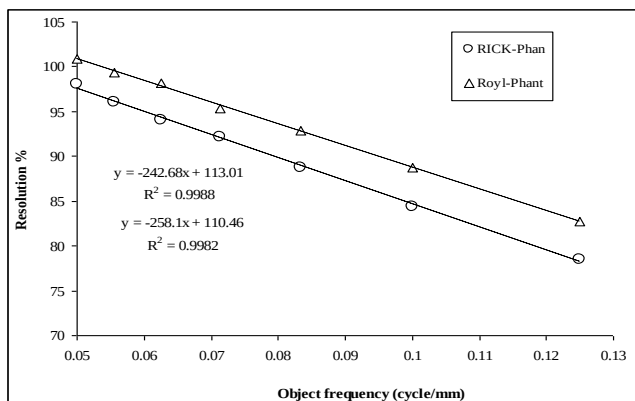


Figure 2: shows the resolution % vs. objects frequency for SPECT in RICK and Royal care hospitals-Khartoum Sudan using developed phantom.

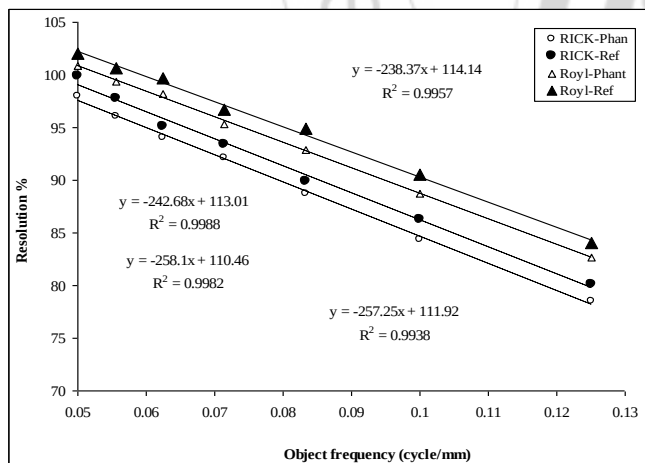


Figure 3: shows the comparison resolution% measured by phantom and the QA base line for Royal Care and RICK hospitals.

4. Discussion

Figure (1) shows the resolution % vs. objects size for SPECT at RICK and RCH-Khartoum Sudan. The analysis reveals that: the resolution percent increases following the objects size increment for both hospitals i.e. RCH and RICK, however RCH and RICK showed the average resolution of 94.0% and 89.5% respectively as measured by the designed phantom relative to the standard resolution measured by the NEMA phantom which was 95.5% and 90.8%, while the correlation between the resolution% and the objects size in mm could be fitted to the following equation $y = 6.59x + 47.87$ and $y = 6.64x + 43.1$ for Royal Care and RICK respectively with significant correlation as $R^2 = 0.98$. The system resolution at RCH has been within the tolerance level i.e. 3-5% from the optimum resolution (100%), however the system at RICK showed an action level which is $> 5\%$ relative to the optimum resolution (100%) as has been mention by IAEA, [15] and Ellinor et al, [2]. Therefore the system installed at RICK should be subjected to serious QC process to reassure the optimum or at least tolerance level of resolution.

Figure 2 shows the comparative resolution % vs. objects frequency for SPECT at RICK and RCH. The analysis showed that: there is inverse linear relationship between the resolution% and the objects frequency (number of wires/cm) i.e. as the frequency increases the resolution% decreases for both hospitals and the average resolution% was 94% and 90.3% respectively as measured by the designed phantom and in comparison with that obtained by NEMA phantom which was 95.5% and 91.8% respectively, the average deviation factor of the designed phantom from the standard was -1.5%. in contrast with the standard ranged of resolution stated by Ellinor et al, [2], both systems installed at RCH and RICK have been shifted from the standard range but the system at RICK was at action level. The correlation between resolution % and the objects frequency could be fitted in equations: $y = -242.68x + 113.01$ for RCH and $y = -258.1x + 110.46$ for RICK, where x refers to objects frequency and y refers to resolution%, such correlation was significant as $R^2 = 1$. The average resolution% measured by the phantom was 94% and 90.3% respectively.

Figure 3 shows the comparison resolution% versus object frequency measured by developed phantom and the QA base line for RCH and RICK. The general trend of the analyzed data showed that: there were inversely linear relationships between object frequency and resolution with significant point at $R^2 = 0.9$ % i.e. as the object frequency increases the resolution% decreases. The average resolution measured by the developed phantom was 94.0% and 90.3% for RCH and RICK respectively, these results relative to the standard NEMA QA phantom which was 95.5% and 91.8% respectively. Same resolution as 94.0% and 89.5% have been obtained for RCH and RICK respectively depending on the resolved object size as shown in Figure (4) which is compared with standard results obtained by NEMA phantom as 95.8% and 91.5% to deduce that: the average shift of the designed phantom relative to standard one was also 1.9%. Hence the developed designed phantom could be use successfully to carry out the QC tests for SPECT in Sudan with an average deviation factor of -1.3% from the optimum resolution measured by NEMA phantom.

5. Conclusion

In case of low budgets or lack of funding to purchasing SPECT system with full option of QC tools, the designed phantom could serves the NM specialist to carry out the resolution QC test successfully and the other tests could be contemplated and verified also with figuring out the deviation factor.

References

- [1] Steven Burrell, and Anita MacDonald. (2006). Artifacts and Pitfalls in Myocardial Perfusion Imaging. Journal of Nucl. Med. Technol. Vol. 34, P: 193–211.
- [2] Ellinor Busemann Sokole, Anna Plachcńska, Alan Britten, M. Lyra Georgosopoulou, W. Tindale and R. Klett. (2010). Routine quality control recommendations for nuclear medicine instrumentation. Eur J. Nucl. Med. Mol Imaging, vol. 37, P: 662–671
- [3] National Electrical Manufacture Association performance measurements of Gamma cameras NEMA standard publication NU 1 – 2007.
- [4] National Electrical Manufacturers Association (NEMA), (2001). Performance Measurements of Scintillation Cameras; NEMA Standards Publication NU 1-2001, Washington, D.C.-USA: Global Engineering Documents.
- [5] O'Connor M. K, Vermeersch C. (1991). Critical Examination of the Uniformity Requirements for Single Photon Emission Computed Tomography. Med Phys vol. 18, P: 190-197.
- [6] Young KC, Kouris K, Awdeh M, Abdel-Dayem HM. (1990). Reproducibility and Action levels for Gamma Camera Uniformity. Nucl. Med Commun; vol. 11, P: 95-101.
- [7] John E. Ejeh, Kayode S. Aedapo, Bidemi I. Akinlade, Bola O. A. Osifo. (2011). Gamma camera intrinsic uniformity in an unstable power supply environment. Hellenic Journal of Nuclear Medicine, vol. 14 (2), P: 1790-5427.
- [8] Abdelhamid A. Elkamhawy, Joseph R. Rothenbach, Srikanth Damaraju, and Shamim M. Badruddin. (2000). Intrinsic Uniformity and Relative Sensitivity Quality Control Tests for Single-Head Gamma Cameras, J. Nucl. Med. Technol. Vol. 28, P: 252–256.
- [9] [9] International Atomic Energy Agency, "Quality control of nuclear medicine instrumentations, IAEA-TECDOC602", 1991.
- [10] Ng A.H., K.H.Ng, H. Dharmendra, A. C. Perkins. (2009). A low-cost phantom for simple routine testing of single photon emission computed tomography (SPECT) cameras. Applied Radiation and Isotopes, vol. 67, P: 1864–1868.
- [11] Holstensson Maria, Mike Partridge, Susan E Buckley and Glenn D Flux. (2010). The effect of energy and source location on gamma camera intrinsic and extrinsic spatial resolution: an experimental and Monte Carlo study. Phys. Med. Biol. Vol.55, P: 1735–1751.
- [12] Holstensson M, Hindrof C, Ljungberg M, Partridge M, Flux GD. (2007). Optimization of energy-window setting for scatter correction in quantitative 111in imaging: Comparison of measurements and Monte Carlo simulations. Cancer Biother. Radiopharm. Vol. 22(1), P: 136-142.
- [13] Islamian Jalil Pirayesh, Mohammad Taghi Bahreyni Toossi, Mehdi Momennezhad, Shahrokh Naseri and Michael Ljungberg (2012). Simulation of a Quality Control Jaszczak Phantom with SIMIND Monte Carlo and Adding the Phantom as an Accessory to the Program. Iranian Journal of Medical Physics, Vol. 9, No. 2, P: 135-140.
- [14] Zanzonico Pat. (2008). Routine Quality Control of Clinical Nuclear Medicine Instrumentation: A Brief Review. J. Nucl. Med. Vol. 49(7), P: 1114–1131.
- [15] IAEA. (2009). Quality Assurance for SPECT system (Human Health Series No. 6), Vienna, Austria.

Author Profile



Mohamed Elfadil M. Gar-el-nabi: awarded B. Sc. in Radiotherapy and Nuclear Medicine, and M.Sc. degrees in Medical Physics from Sudan University of Science and Technology in 1995 and 2001 respectively. He has been working as medical physicist and radiation therapy specialist at Radiation and Isotopes Center of Khartoum as well as a lecturer at College of Medical Radiologic Science, Sudan University of Science and Technology. He received a Ph. D. degree from Natal University South Africa - 2007 in Medical physics and now working as a lecturer (Associate Prof.) at Sudan University of Science and Technology-Khartoum-Sudan.



Wadah Mohammed Ali: Award B. Sc. Degree from the National Ribat University in Nuclear Medicine 2007, M. Sc. from Sudan University of Science and Technology in Nuclear Medicine 2010 and M. Sc. in Radiation Protection & Environmental Science from Sudan Academy of Science (SAS) 2015. He has been working as NM specialist at Radiation and Isotopes Centre of Khartoum RICK during 2007-2010 and a lecturer in National Ribat University since graduation till now.



Mohammed Ahmed A. Omer: received the B. Sc. -1. in Radiotherapy and Nuclear Medicine, B. Sc.-2 in Medical Equipments Technology and M.Sc. degrees in Medical Physics from Sudan University of Science and Technology in 1995, 1998 and 2001, respectively. He has been working as radiation therapy specialist and medical physicist at Radiation and Isotopes Center of Khartoum (1995-2003) as well as a lecturer at College of Medical Radiologic science-Sudan University of Science and Technology. He awarded a Ph. D. degree from University Putra Malaysia - 2007 in Medical physics-Applied Radiation and now working as a lecturer (Associate Prof.) at Al-Qassim University-Buraidah-KSA.



Ghada Abker Edam Sakin: Awarded B. Sc. Degree in Nuclear Medicine in 2010 from National Ribat University-Sudan and M. Sc. from College of Medical Radiologic Science-Sudan University of Science and Technology 2013. She has been working as a lecturer (part timer) at Sudan University of Science and Technology department of Radiotherapy and Nuclear Medicine since up to 2013. Now she is a Ph. D. candidate in same field

